


Out of Darkness

Helping the blind see with artificial vision.



Vision impairment is a major disability faced by millions around the world. Right now, the only way to obtain information about the world, reading, and enjoy life, and thus the ability to work, is through the use of a white cane. However, several groups around the world have used principles of electrical vision systems based on the principle of electrical activation of the retina (EAV). The retina is composed of multiple layers of neurons (i.e., microcircuits), electrically connected to each other. In a healthy eye, photoreceptors are stimulated by light, which photoreceptors are attached to. Because the eye loses the ability to sense light when photoreceptors are attacked by disease, the eye loses the ability to sense light. Current research focuses on how to bypass this loss of light by using electrical stimulation. These systems typically consist of an image sensor, integrated circuits to generate stimulation pulses, and a way to connect the implanted circuitry, and a flexible, low-dimensional microelectrode array, which is implanted directly to apply an electrical stimulus to the retina. As shown schematically in Figure 1, current prototype systems all have several components that are essential to the system, including an image sensor, camera, inductive energy transfer system to wirelessly power the system, and data collection hardware to allow wireless programming of the system. In recent years, each of these early prototype devices has demonstrated increased mobility and improved performance in visually guided tasks.

James D. Weiland, Mark S. Flanagan, and Armand K. Engert Jr.

Recent advances in the ability of EAV to be used by active implants, as low power systems that can be implanted in the eye, and system efficiency, have inspired several groups to design or technology, from low power is available for retina stimulation. The energy systems could employ low power technology to manage power usage to that the greatest degree to avoid a large battery. Gene Vitaz has worked with our team for more than 12 years to develop the power technology within these systems (1) that could benefit retina prostheses. 1) low power digital signal processing circuitry could be the external vision processing unit of a retina prosthetic.

Digital Photo: Andrew J. G. Jones/ISTOCKPHOTO
Photo: iStockphoto.com/1234567890
www.istockphoto.com/1234567890
www.istockphoto.com/1234567890

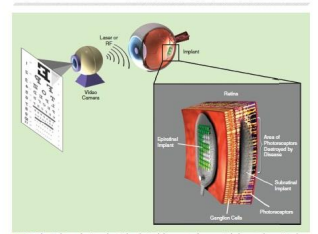


FIGURE 1. Schematic diagram of an artificial eye system. An external camera captures an image of the world, which is transmitted wirelessly to an external transmitter. The transmitter sends signals to an external receiver, which is implanted in the eye. The receiver is connected to a retinal implant that stimulates the retina. Labels include: Camera, Transmitter, Receiver, Retinal Implant, and Retina.

Several groups around the world have tested prototypes of artificial vision systems based on the principle of electrical activation of the retina.

Products Argus II Retinal Prosthesis, which was recently approved for sale in Europe. Research collaborations between the Neurosciences, Microelectronics Systems Engineering and Research Center (MERC) at the University of Southern California (USC) have focused on advanced technology for future biomedical systems, including the development of an electrical circuit to replace the external camera and provide for the natural coupling of head and eye movements.

Current microelectrode technology is insufficient to activate the retina, which necessitates a continuous external power supply, which an implanted battery would not have the necessary capacity to power an implant without frequent recharging. Future advances in microelectrode array technology will allow closer contact between the implant and the retina, which may reduce the need for external power.

The low power digital signal processing circuitry could be the external vision processing unit of a retina prosthetic. This technology could be used to process the image data from the external camera and provide for the natural coupling of head and eye movements.

Current microelectrode technology is insufficient to activate the retina, which necessitates a continuous external power supply, which an implanted battery would not have the necessary capacity to power an implant without frequent recharging. Future advances in microelectrode array technology will allow closer contact between the implant and the retina, which may reduce the need for external power.

