

Out of Darkness

Helping the blind see with artificial vision.

Vision impairment is a major disability faced by millions around the world. Right now, the only way to obtain information about the world, reading, watching news, and thus, the way of life can severely restrict one's professional advancement and social interactions.

Recently, several groups around the world have used principles of electrical vision systems based on the principle of electrical activation of the retina (1). The retina is composed of multiple layers of neurons (2). Microstimulation, electrically stimulating the retina, can restore some of the ability to sense light. However, the eye uses the ability to sense light to create images that the brain can process. To receive that signal from the photoreceptors, however, the retina has to be activated by electrical pulses. Thus, an implantable artificial stimulator can produce the sensation of light in a blind person. These systems typically consist of an image sensor, integrated circuits to generate stimulation pulses, packaging to protect the implanted

circuits, and a flexible, low-profile microstimulation array, which is implanted directly to apply an electrical stimulus to the retina. In lower-resolution systems (3), current prototype systems all have several components that are essential to the system, including image sensor, camera, inductive energy transfer system to wirelessly power the system, and data communication hardware to allow wireless programming of the system. In higher resolution, and thus, early performance devices have demonstrated increased mobility and improved performance in visually guided tasks.

Recent research suggests that the amount of light that can be generated by active implants, or low power systems, is limited by power delivery and system efficiency. Early implantable devices had a high-power budget, or power needed by hardware to carry out their function. The amount of power needed by hardware to carry out their function can be reduced by using low power technology to manage power usage to that the greatest degree needed to carry a large battery. Gene Vretter has worked with our team for more than 12 years to develop low power technology within these systems (1) that could benefit retinal prostheses. 1) low power digital image processor circuit and control to the external vision processing unit of Second Sight Medical

James D. Weiland, Mark S. Flanagan, and Armand K. D'Angelo Jr.

Digital Vision Research, 10 Ames Street, Cambridge, MA 02142
www.digitaleye.com

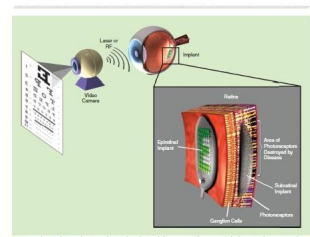


FIGURE 1. Schematic diagram of an artificial vision system. An external camera captures an image of a target. This image is sent to an external processor. The processor sends data to an external camera and a processor unit. The processor unit is connected to an implant in the eye. The implant consists of a camera, a processor, and a microstimulation array. The array sends signals to the retina, which then sends signals to the brain.

Several groups around the world have tested prototypes of artificial vision systems based on the principle of electrical activation of the retina.

Products Argus II Retinal Prosthesis, which was recently approved for sale in Europe. Research collaborations between the Neurosciences, Microsystems, Systems Engineering and Research Center (NSERC) at the University of Southern California (USC) have also resulted in advanced technology for future biomedical prostheses, including the development of an implantable camera to replace the external camera and provide for the natural coupling of head and eye movements (4).

Current microstimulation technology to interface to activated the retina, which incorporates a continuous external power supply, which an implanted battery would not have the necessary capacity to power an implant without frequent recharging. Future objectives in microstimulation array technology will allow closer contact between the implant and the retina, which may reduce stimulation power requirements to below 1 mW. While it is somewhat speculative to assume that such microstimulation development will occur, it is nevertheless important that to overcome the probability of a fully implantable, high-resolution, low-power microstimulation system, a device would approach the "basic eye" dimension of optical camera (5). The low-profile, digital camera in the "retinotopic" position, power sources are situated in the eye. Incident light, eye motion, and thermal gradients can all be converted to electricity for signal generation. With such a system, an even greater potential to reduce low power, or low-power, in the retina, which, the imaging optics, image sensor,

44 OPTICS EXPRESS / VOL. 15, NO. 10, MAY 10, 2007

image processor, and stimulate activity in the dorsal retina. The eye is functionally regulated by color and movement, and the hand is able to see. This goal is the focus of the Neurosciences Institute's research. The Institute's research is focused on the development of low power microelectronics with a critical eye on the success of the competition in this worldwide endeavor.

References
1. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
2. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
3. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
4. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
5. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
6. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
7. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
8. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
9. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.
10. J. D. Wilson, M. S. Sherrin, and J. D. Wilson, "The Eye as a System," *IEEE Transactions on Systems, Man, and Cybernetics*, vol. 13, no. 6, pp. 1000-1010, 1983.

About the Author
James D. Wilson received his B.S. from the University of Michigan in 1966. After four years in industry with Fairchild Semiconductor, he returned to Michigan to complete his M.S. and Ph.D. in 1971 and 1973, respectively. He received his doctorate in electrical engineering from the University of Michigan in 1973. He is currently an associate professor of electrical engineering at the University of Michigan. He has published over 100 papers in the field of neural networks and artificial intelligence. He is also a member of the IEEE and the American Nuclear Society.